7000BY QUICK INSTALLATION GUIDE
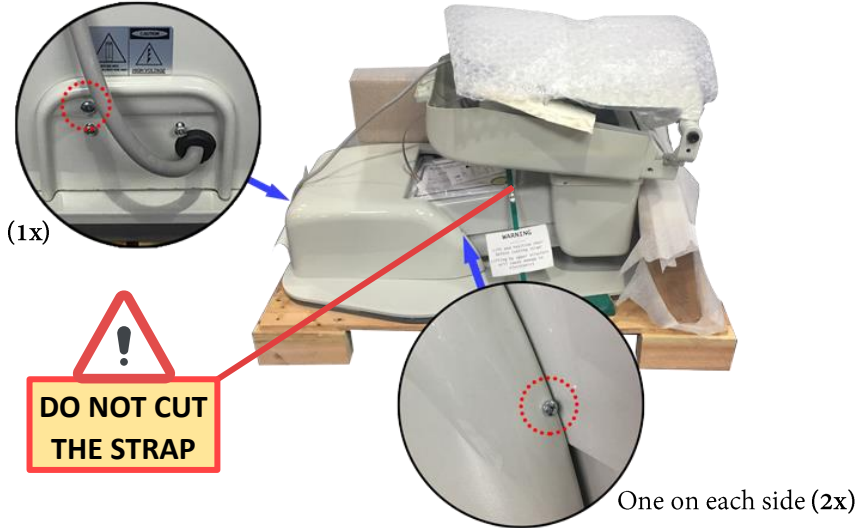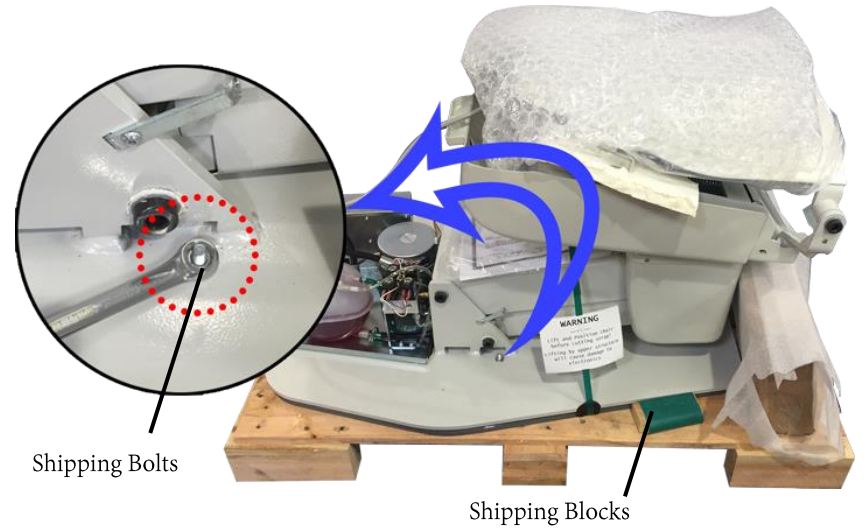
1 After removing the box from the pallet. Remove the pump cover via 3 Philips screws.
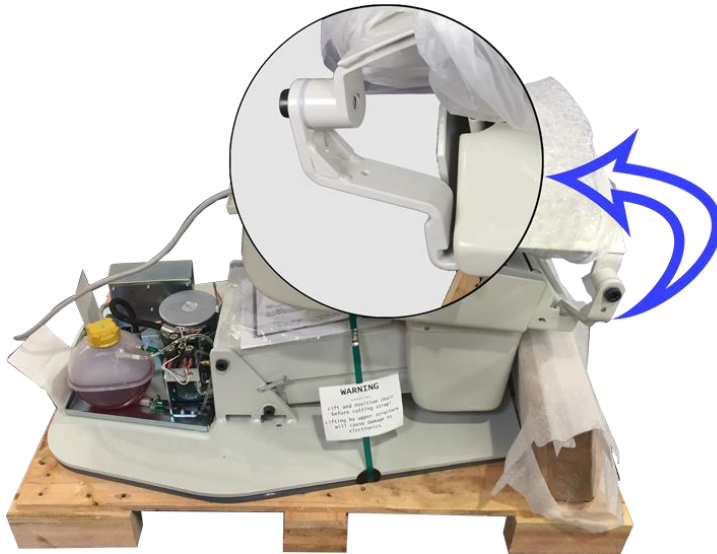
(1x)

DO NOT CUT THE STRAP

One on each side (2x)

2 Using a ½" wrench, remove shipping bolts. Remove shipping blocks.
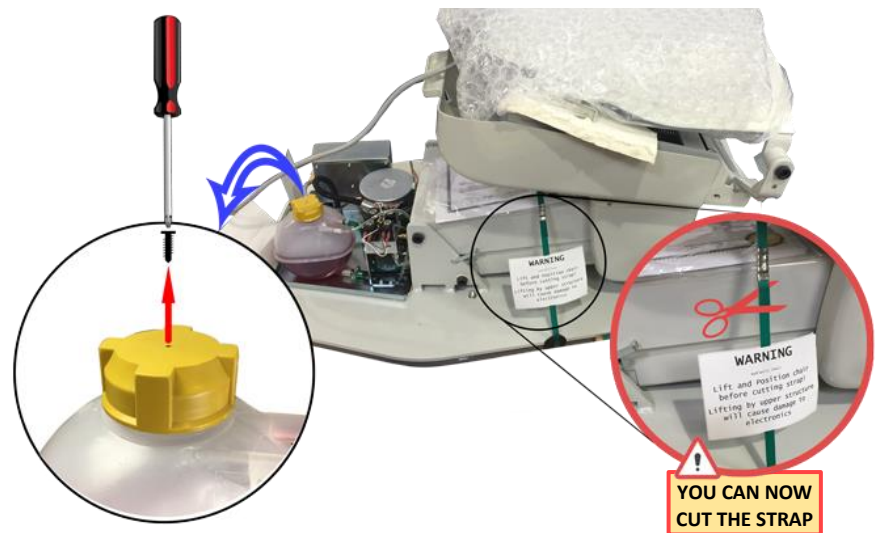
Shipping Bolts

Shipping Blocks

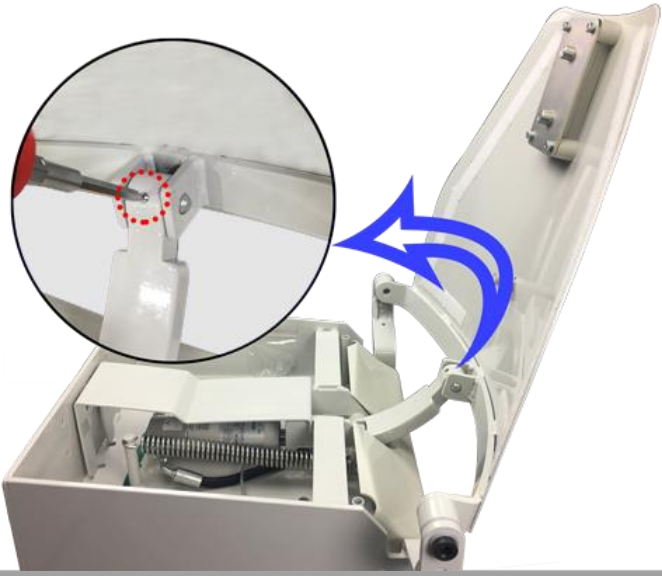**3** Lift the chair off the pallet using the backrest/armrest mounting brackets.

4 Once the chair is positioned in its final location, cut the strap and remove the shipping screw from the reservoir cap.

WARNING

Lift and Position chair before cutting strap. Lifting by upper structure will cause damage to electronics.

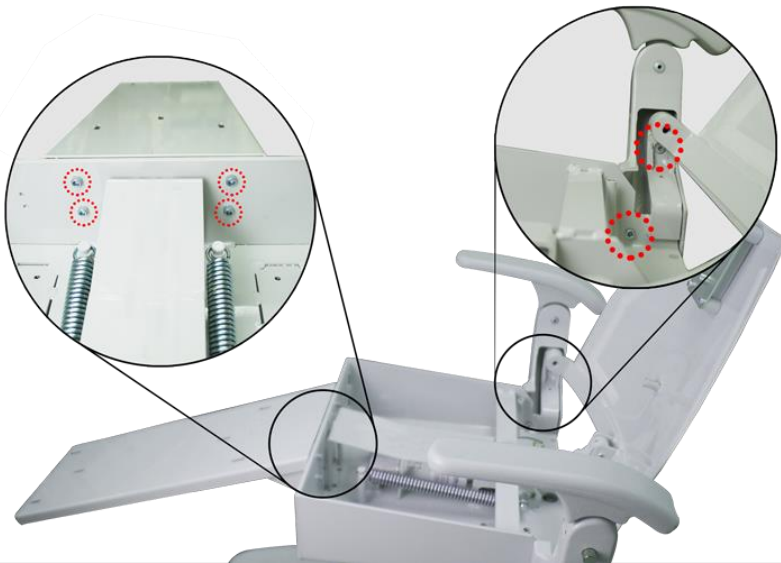**YOU CAN NOW CUT THE STRAP**

7000BY QUICK INSTALLATION GUIDE

5 Raise base to full up position, lift backrest, install pin, and tighten set screw.

6 Remove back piston cover.

7 Install toe pan and armrest.

8 Install upholstery, re-install all covers and test all chair functions.

SDS
Summit Dental Systems